

**FIG. 1**

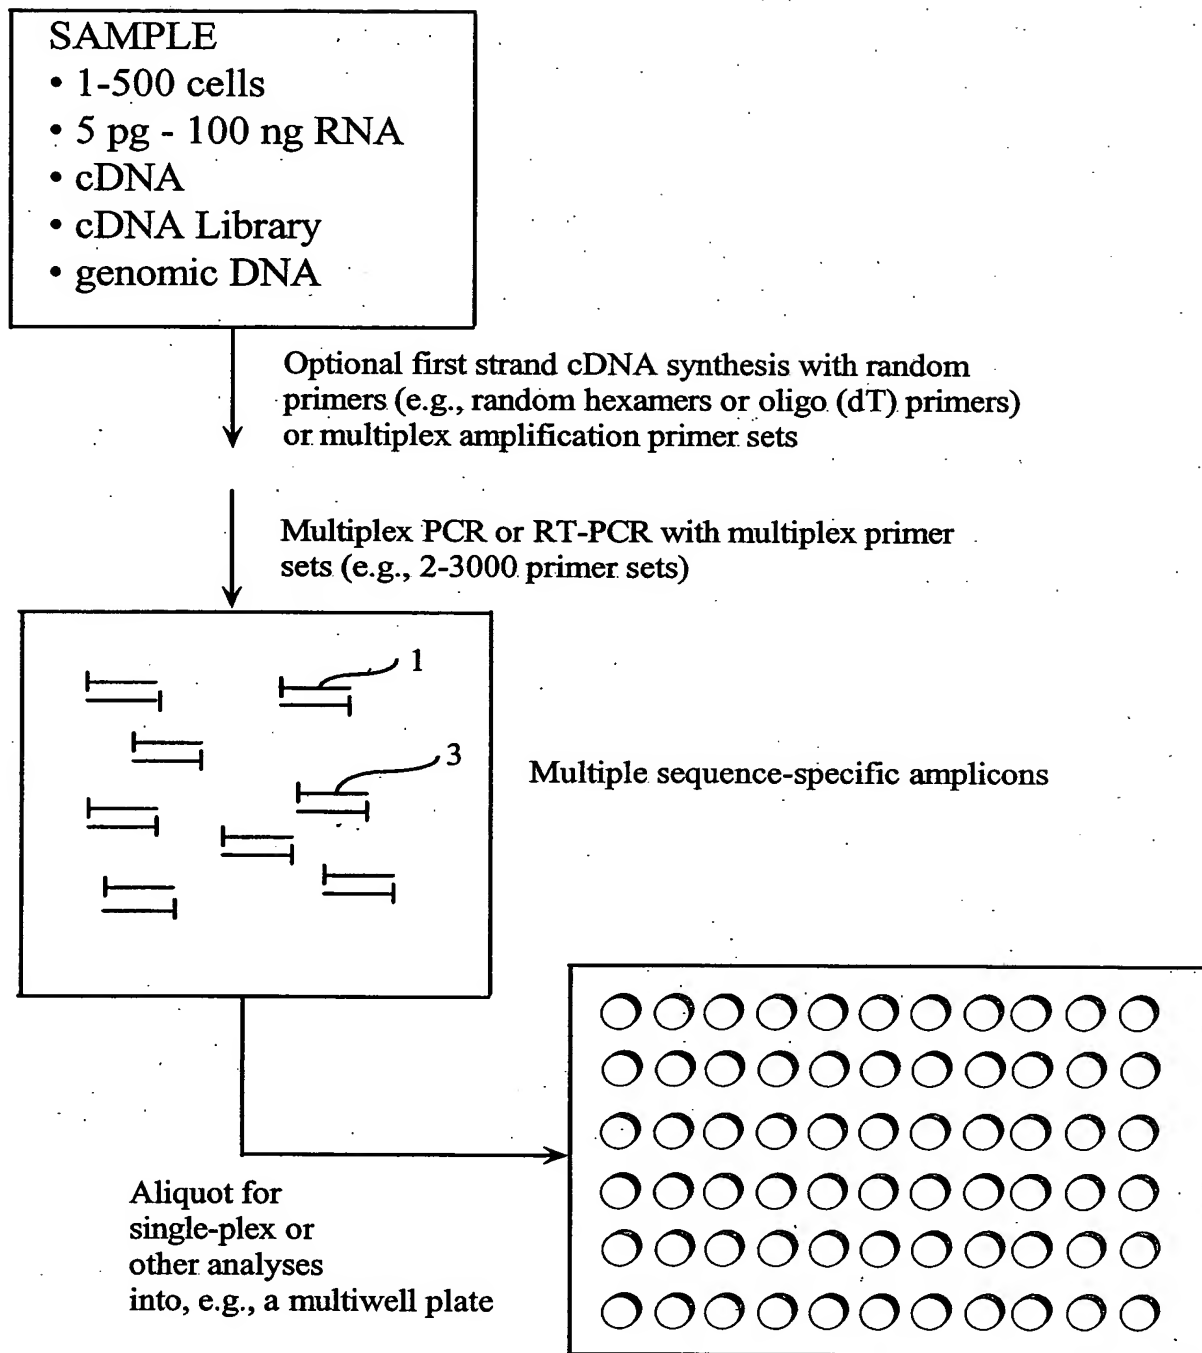


FIG. 2

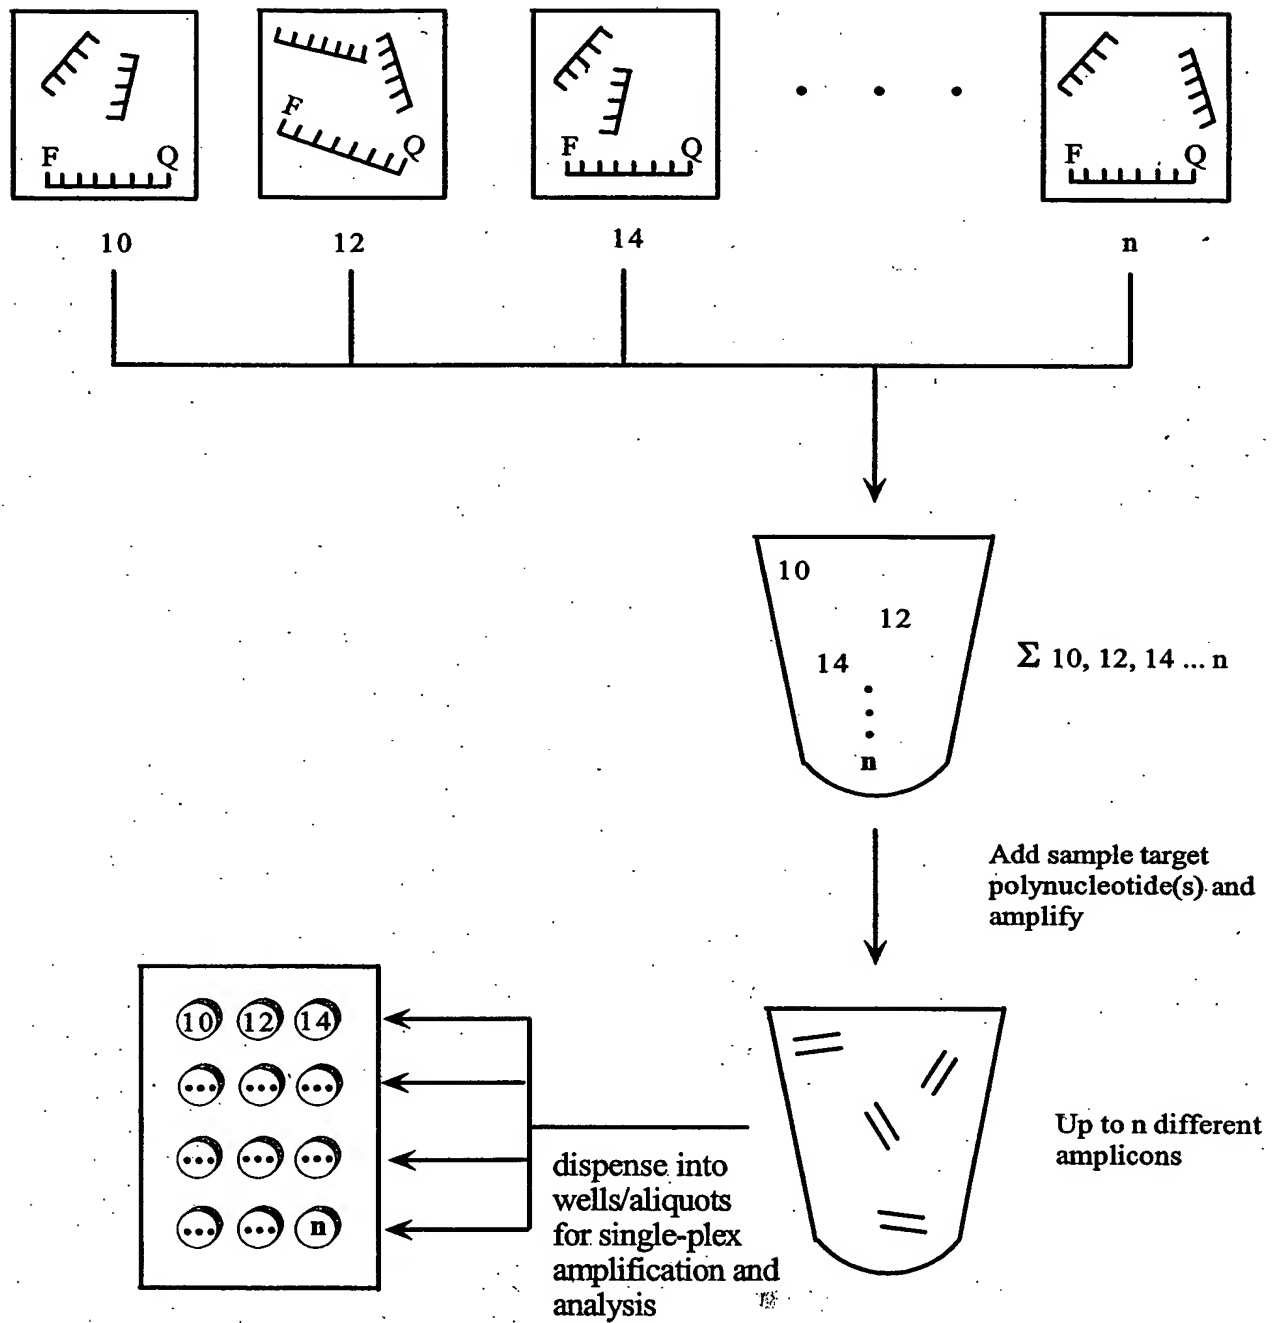
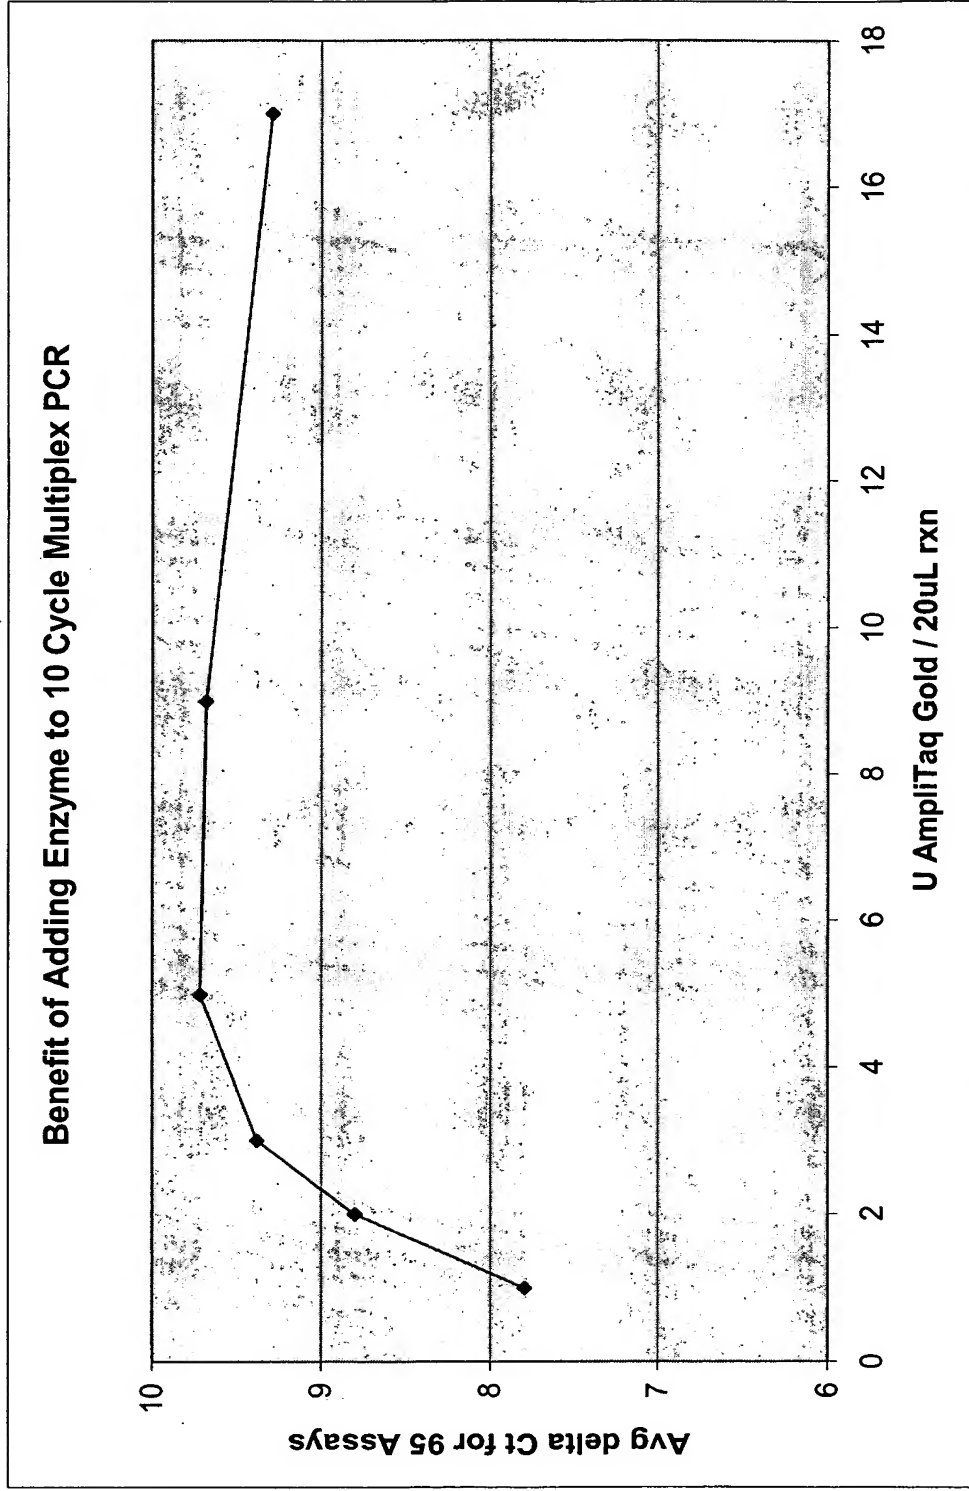


FIG. 3



**FIG. 4**

**Efficiency of 10 Cycle Multiplex**

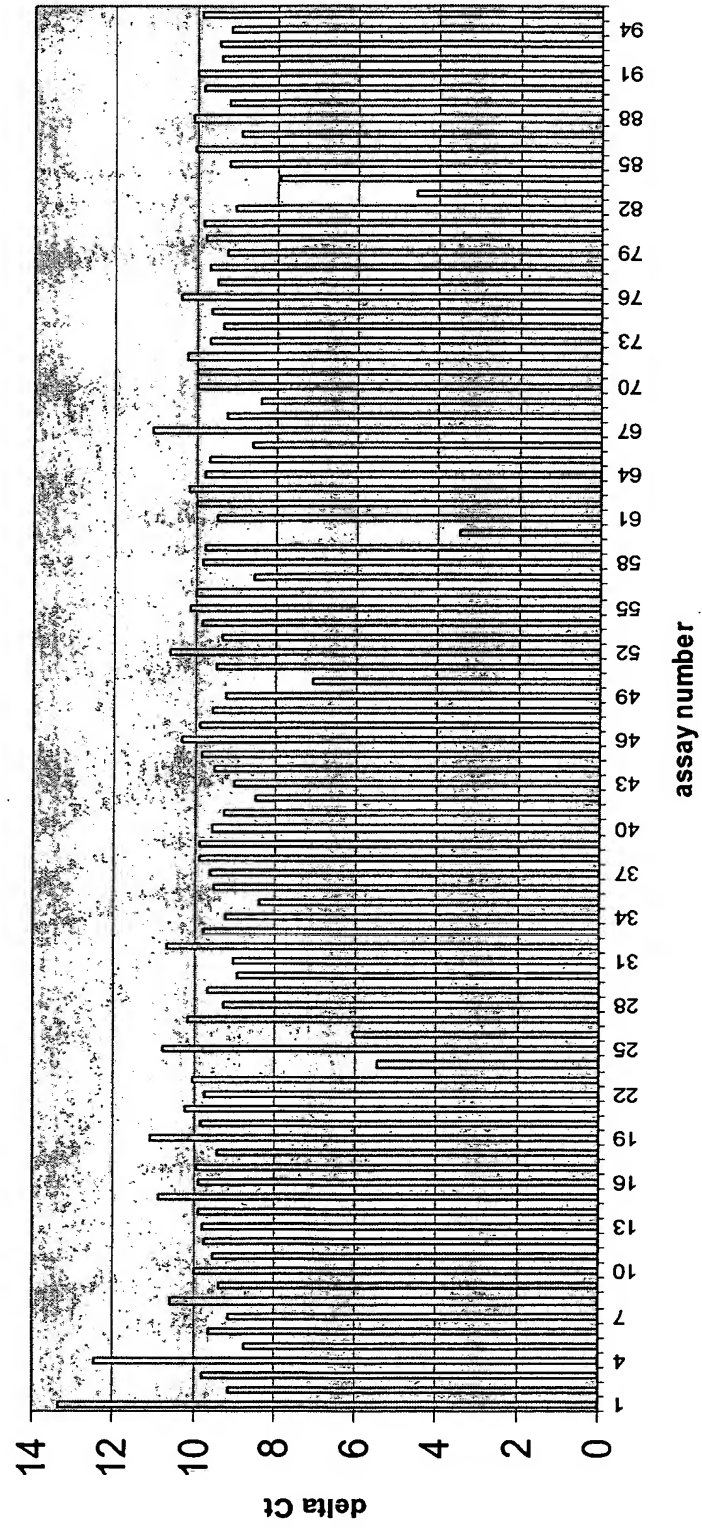


FIG. 5


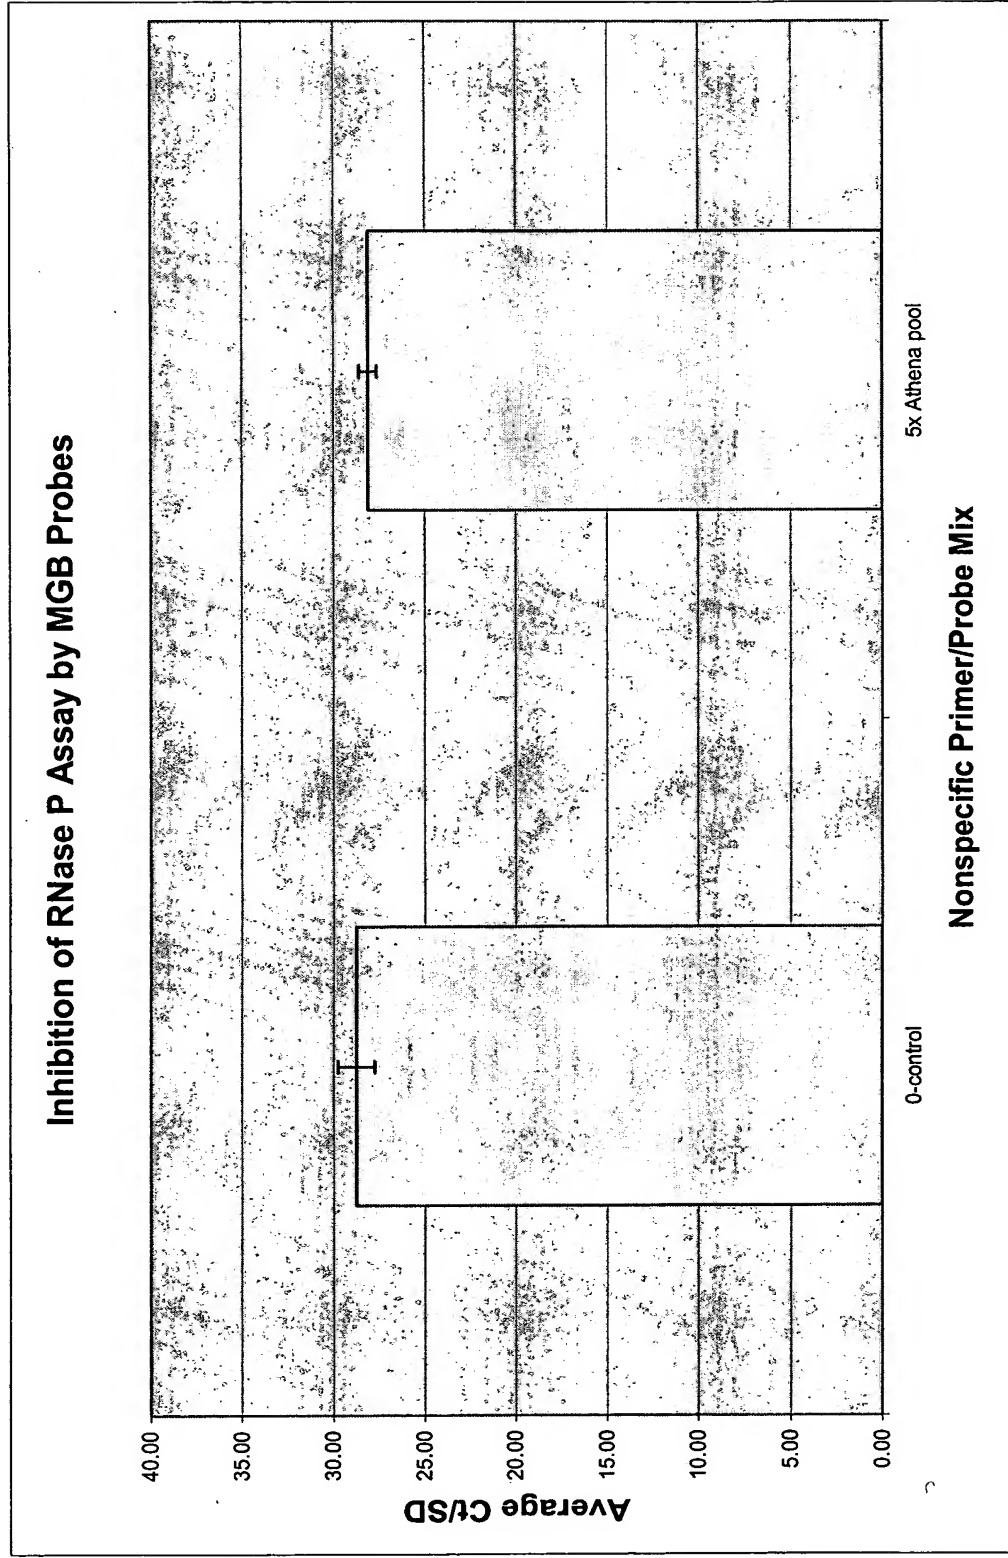


FIG. 6  
Titration of cDNA

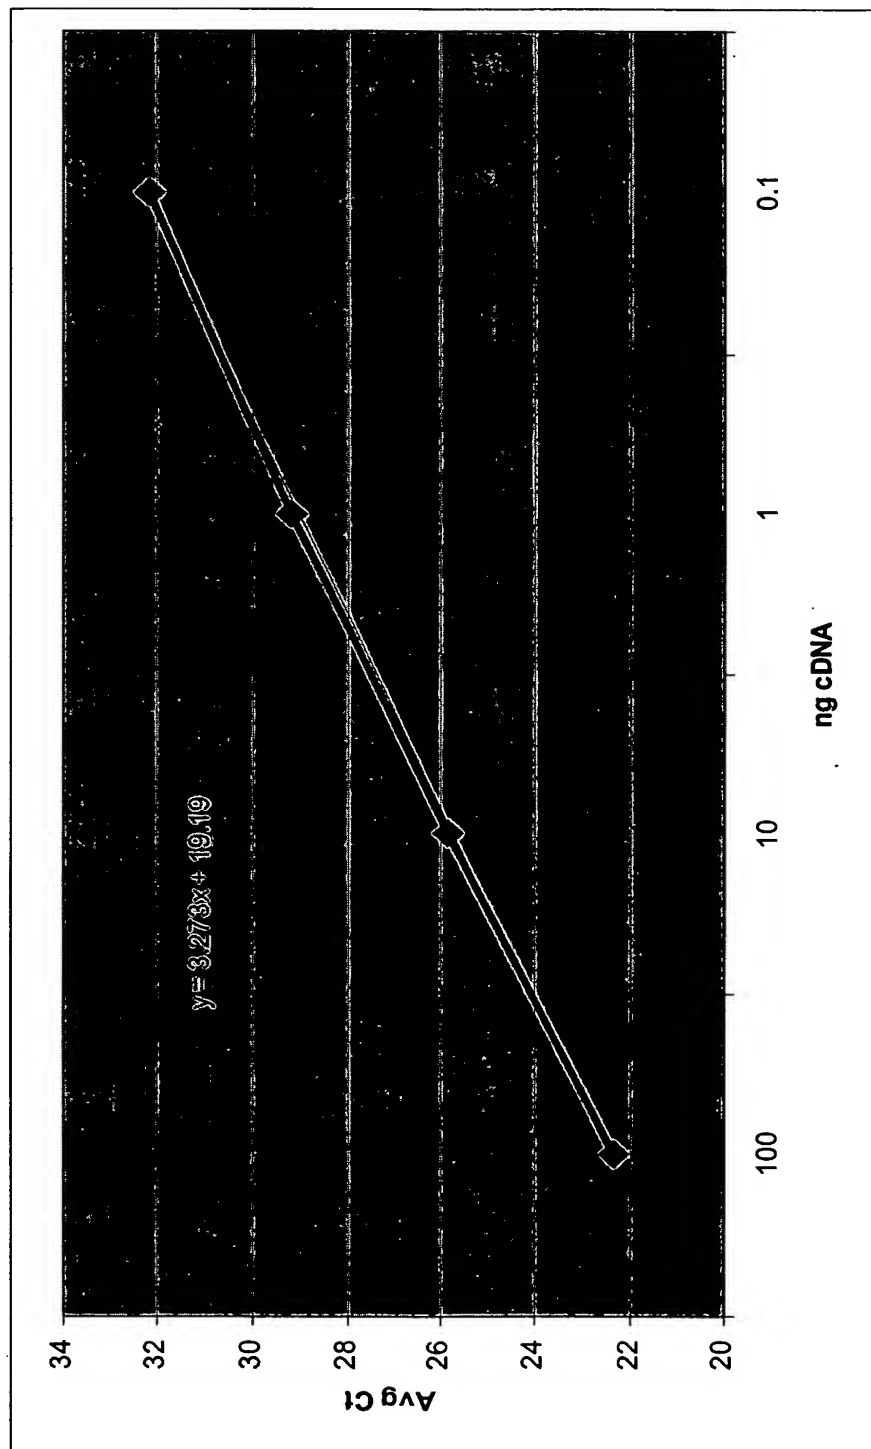

Sorted by Delta Ct (common assays with mock <38): preamp 94-plex to 1013-plex

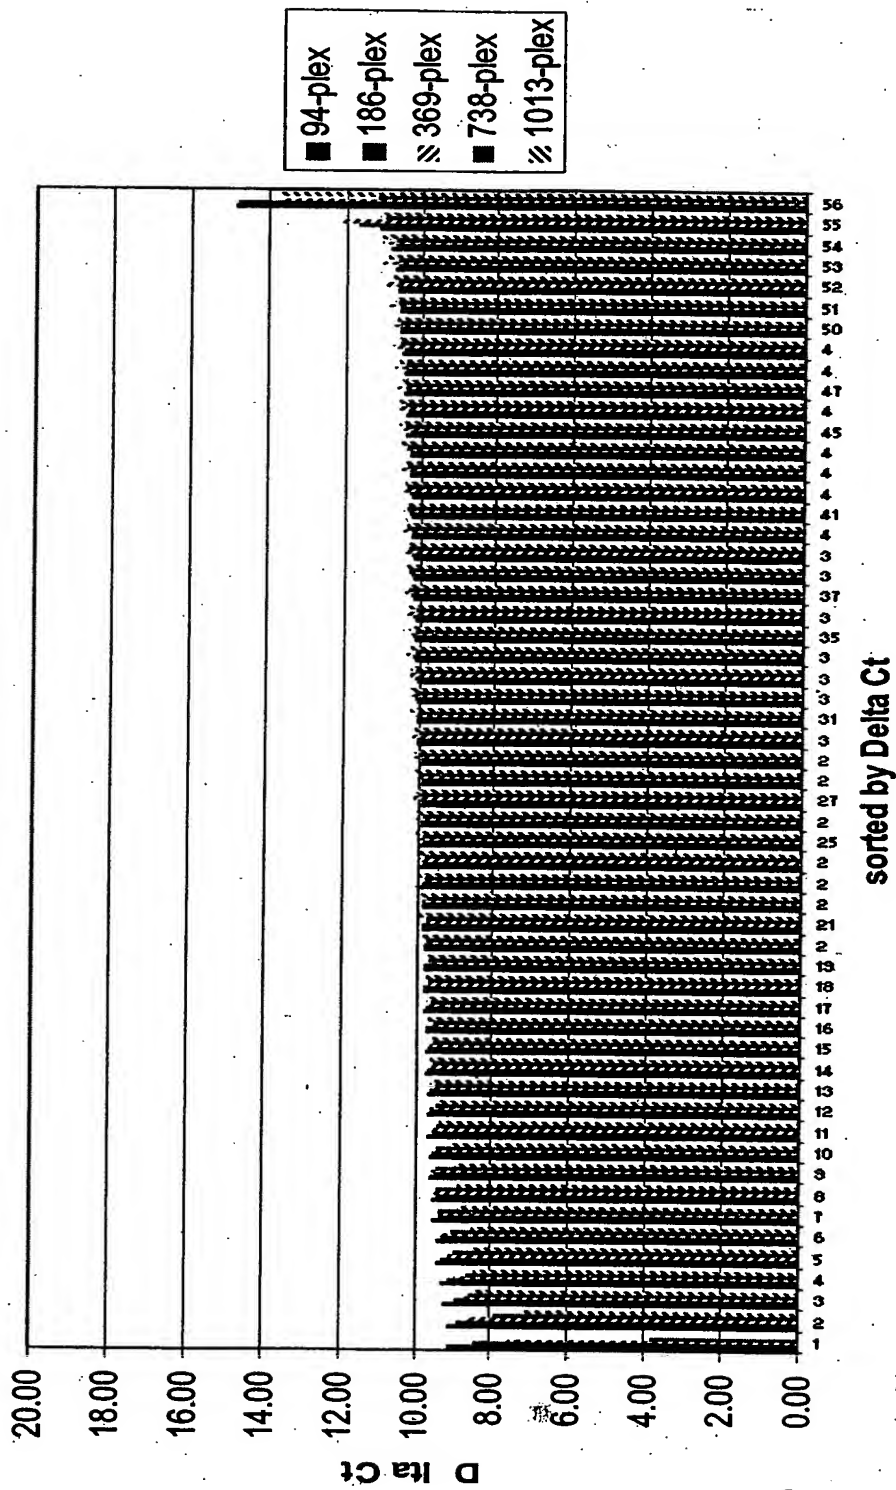


FIG. 7

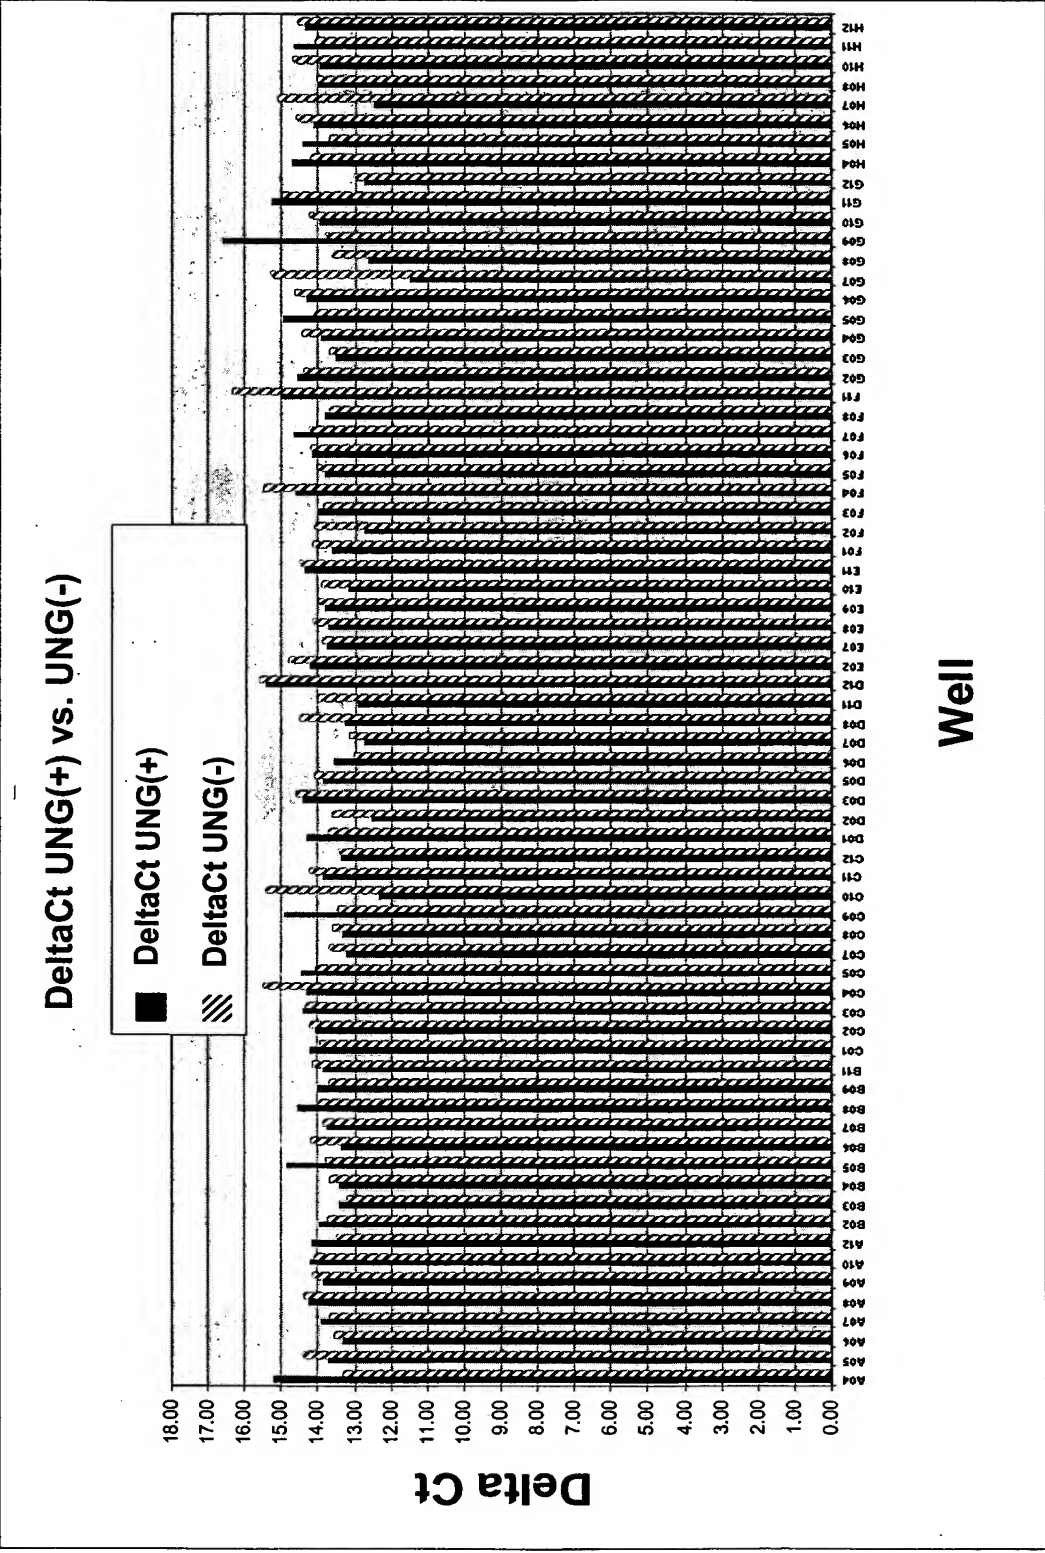


FIG. 8



delta Ct values for 10-14 cycles of preamp: IAP assays

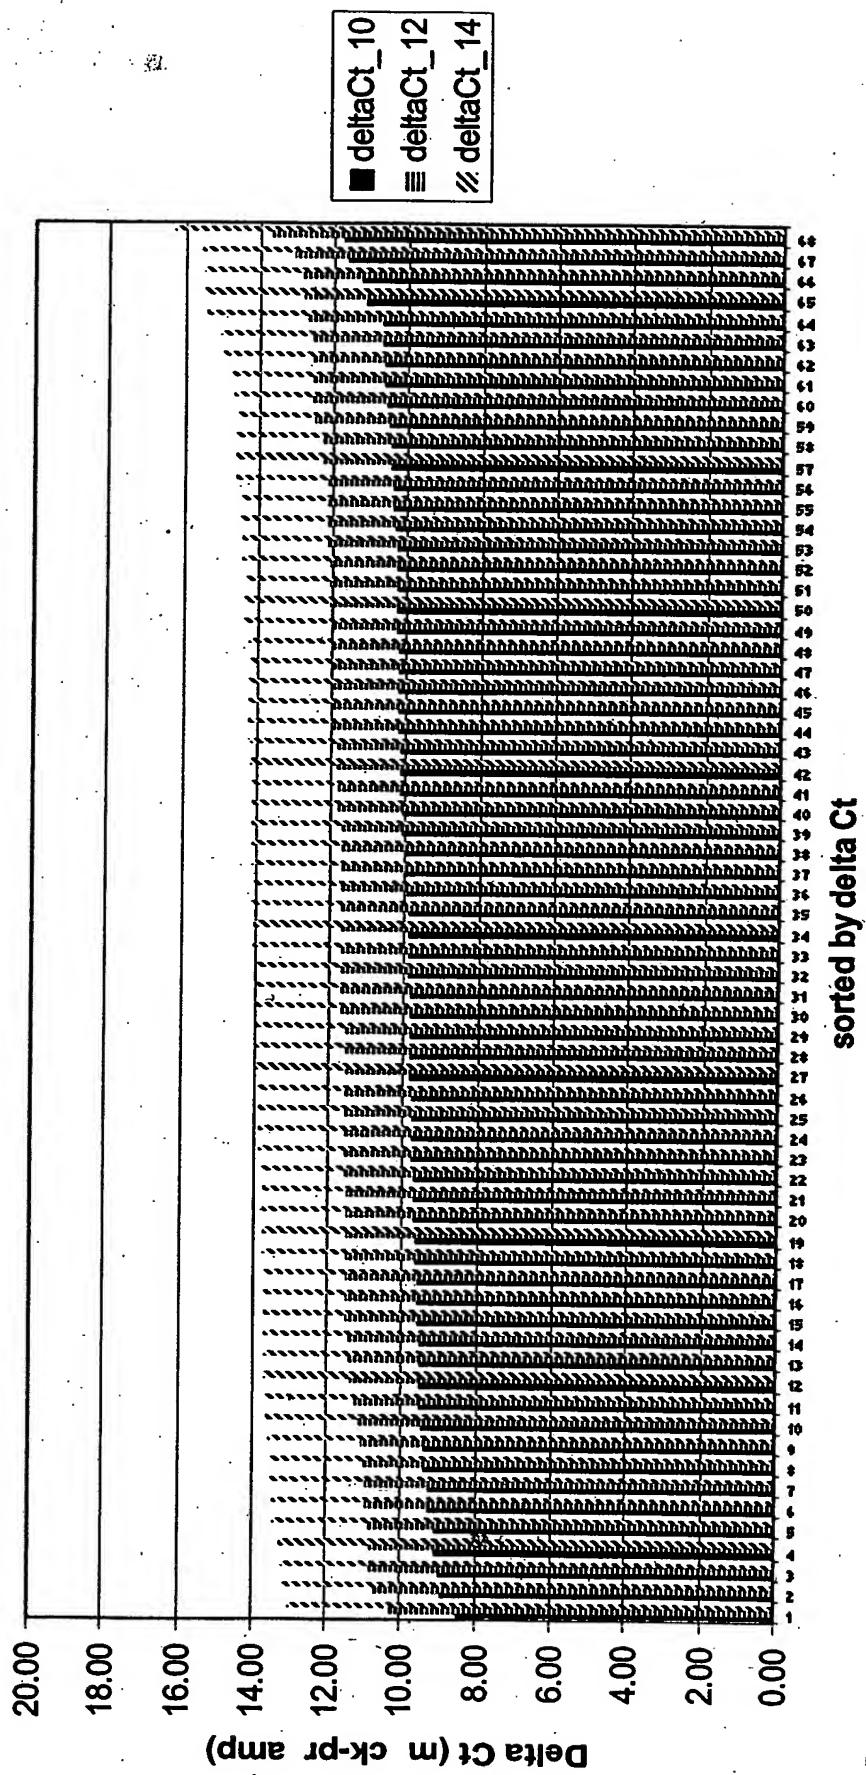


FIG. 9